### Omnia pure and ultrapure water systems Convenient. Compact. Adaptable.





### H<sub>2</sub>O pure. Pure and ultrapure water For QC, R&D and analytical labs in science, pharmaceutics and industries.

Whether for demanding applications in life sciences and chemical analysis or for supplying analysers, autoclaves and laboratory glassware washers – with seven systems, the new stakpure Omnia series provides the ideal solution for any task and satisfies international water standards such as ASTM, ISO 3696 and CLRW (CLSI). The systems are characterized by their economy and flexibility in many applications.

					OmniaLab <sup>ED+</sup>	
	OmniaTap	OmniaPure	OmniaLab <sup>ED+</sup>	OmniaTap	OmniaLab <sup>ED</sup> OmniaLab <sup>UP</sup> OmniaLab <sup>DS</sup>	OmniaLab <sup>RO</sup>
Water quality		Type I ultrapure water			vpe ll 9 water	Type III water from reverse osmosis
daily water quantity	< 50 liter	20–100 liter	> 50 liter	< 50 liter	> 50 liter	> 50 liter
feedwater	tap water	pretreated water	pretreated water	tap water	pretreated water	pretreated water
applications	<ul> <li>IC (Ion Chromate</li> <li>ICP (Inductively 6</li> <li>ICP-MS (Inducti</li> <li>ICP-MS (Inducti</li> <li>HPLC (High-perf</li> <li>HPLC + (Ultrates)</li> </ul>	Coupled Plasma) vely Coupled Plasma Mass ormance liquid chromato ce Element Analysis) and Electrophoresis		<ul> <li>Reagent Prepara Sample Dilution</li> <li>Buffer and medi</li> <li>Photometry + Sp</li> <li>RIA (Radioimmu</li> <li>ELISA (Enzyme-li immunosorbent</li> <li>Pathology + Hist</li> <li>General chemist</li> <li>Feeding of ultrap</li> <li>laboratory was</li> <li>autoclayes + st</li> </ul>	a preparation pectrophotometry noassay) nked assay) ology ry pure water systems: hers (OmniaLab)	<ul> <li>Feeding of ultrapure water systems:         <ul> <li>laboratory washers</li> <li>autoclaves</li> <li>sterilizers</li> <li>steam generator</li> <li>climatic chamber</li> </ul> </li> </ul>

### Water quality standards For various fields of use and requirements.

#### International Organization for Standardization (ISO)

ISO 3696:1987 distinguishes between three degrees of purity for water for analytical purposes in laboratories.

Parameter	Grade 1	Grade 2	Grade 3
pH value at 25°C	_	_	5.0-7.0
Conductivity (µS/cm at 25°C)	0.1	1.0	5.0
Oxidizable matter,		0.00	0.4
oxygen content (mg/l, max.)	-	0.08	0.4
Absorption at 254 nm			
and a lenght of 1 cm	0.001	0.01	_
(absorption units, max.)			
Residue after evaporation by heating to		1	2
110°C (mg/kg, max.)	-	Ι	Z
Silicon content (mg/l, max.)	0.01	0.02	_

#### **Clinical Laboratory Standards Institute (CLSI)**

This institute defined the quality requirements of water for clinical laboratories. The regulations that were valid up to 2006 (NCCL types 1, 2 and 3) but were then invalidated by the requirement that water must be suitable for the intended usage. Only the degree of purity of so-called "Clinical laboratory reagent water" (CLRW) is described.

Parameter	CLRW
Resistance	10 MΩ x cm
ТОС	< 500 ppb
Bacteria	< 10 CFU/ml
Particle content	Inline 0.2 µm-filter

#### American Society for Testing and Materials (ASTM)


The ASTM D1193-06 (2011) deals with the requirements for chemical analyses and physical tests.

er Pure water Ultrapure Water	(μS/cm), max. 0.056 0.056 0.056 0.056 1.0 1.0	(MΩ x cm), min. 18.0 18.0 18.0 18.0 18.0 1.0	- - - -	(μg/l), max. 50 50 50 50	(µg/l), max. 1 1 1	(µg/l), max. 1 1 1	(µg/l), max. 3 3 3	(CFU/ml), max. - 10/1000	(EU/ml), max. - 0.03
Image: state of the state o	0.056 0.056 0.056 1.0	18.0 18.0 18.0		50 50	1 1 1	1 1 1	3		
Image: state of the state o	0.056 0.056 1.0	18.0 18.0	-	50	1	1			0.03
Image: state of the state o	0.056 1.0	18.0	_		1	1	3		
Image: state of the state o	1.0			50			5	10/100	0.25
B B		1.0			1	1	3	100/10	-
B B	1.0		—	50	5	5	3	_	_
B B		1.0	-	50	5	5	3	10/1000	0.03
C	1.0	1.0	_	50	5	5	3	10/100	0.25
ي ااا	1.0	1.0	-	50	5	5	3	100/10	_
	0.25	4.0	-	200	10	10	500	_	-
V Mater	0.25	4.0	-	200	10	10	500	10/1000	0.03
Pure y	0.25	4.0	-	200	10	10	500	10/100	0.25
LIII C	0.25	4.0	-	200	10	10	500	100/10	-
IV	5.0	0.2	5.0-8.0	-	50	50	_	_	-
A Al	5.0	0.2	5.0-8.0	-	50	50	_	10/1000	0.03
Pure N B	5.0	0.2	5.0-8.0	-	50	50	_	10/100	0.25
E IV C	5.0	0.2	5.0-8.0	_	50	50	-	100/10	_

\* Using an appropriate 0,2 µm membrane filter.

### Omnia Pure and ultrapure water systems Convenient. Compact. Adaptable.

### OptiFill Dispenser is standard

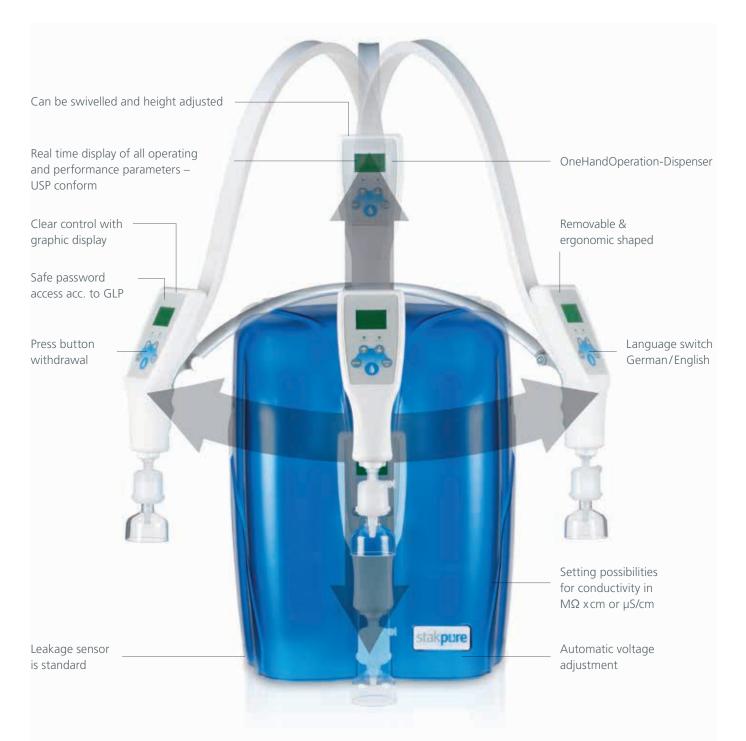

The Omnia series is extremely convenient to use. All devices are fitted with the Optifill one-hand dispenser with integrated control- and monitoring unit. One-handed operation, removable, can be swivelled and height-adjusted, and with a flexible connection for easy water dispensing into any type of container.



The ergonomic shaped dispenser is easily operable.



The easily accessible control and service cover ensures that consumables can be replaced in seconds.

Separate from the production unit. The external dispenser can be space sparingly wall-fitted or flexibly placed on the lab bench.

Place the production unit under the bench to save valuable space in your lab. Match the positioning to your lab environment with the external OptiFill stand/wall dispenser and monitoring unit. Either practical on a bench or space-saving on a wall.



### **OmniaPure** The specialist. For H<sub>2</sub>O pure type I.

When your need is for highest quality pure water that fulfils the demands of analytical and life science laboratory requirements, then one of these OmniaPure systems type will be right for you. You can configurate it. The incorporated pre-treatment constantly ensures the reliability of your experimental results and reduces running costs.

+ Real time TOC monitoring

#### **Features**

- OptiFill dispenser is standard
- Spent filters are simply and quickly changed
- Leakage sensor is standard
- Integrated pressure reducer is standard
- Precise volume control
- Ready-to-use, including filter cartridges









Fits neatly







Dispenser on

the wall






Specificati	ions		OmniaPure	Omnial	Pure UV UV	-TOC	OmniaPure UV/UF	UV-TOC/UF
Туре І								
Conductivi	ty µS/cm		0.055		0.055		0.055	
Resistance MΩ x cm		18.2		18.2		18	.2	
TOC-value <sup>3</sup>	* ppb		5-10		1-5		1-	5
TOC monit	or		-		– / yes		— / y	es
Dispensing	performance l/min.		up to 2		up to 2		up to	1.6
Endotoxins	* EU/ml		-		-		< 0.0	001
RNase* ng/	/ml		-		-		< 0.	01
DNase* pg	/µl		-		-		<	4
Particles**/	/ml		< 1		< 1		<	1
Bacteria**	CFU/ml		< 0.1		< 0.1		< 0	.1
Feedwate	r requirements							
	ared by ion exchange, isation or distillation	, reverse osmo	sis,					
Feedwater temperature °C		+2 up to 35		+2 up to 3	5	+2 up	to 35	
Input conductivity µS/cm		< 30		< 30		< 3	30	
TOC-value	ppb		< 50		< 50		< [	50
Technical o	data							
Operating	pressure bar		0.5 – 6		0.5 – 6		0.5	- 6
Supply volt	age Volt/Hz		90-240/50-60		90-240/50-	60	90-240	/50-60
Connected	load kW		0.1		0.1		0.	1
Connector	size		3/4 "		3/4 "		3/4	ļ "
Ambient te	emperature °C		+2 up to +35		+2 up to +35		+2 up t	:0 + 35
Dimensions	s*** W x H x D mm		390 x 720 x 525		390 x 720 x 525		390 x 72	0 x 525
Dimensions W x H x D i	s production unit mm		390 x 480 x 380		390 x 480 x 380		390 x 48	0 x 380
Dimensions	s OptiFill Wall dispense	er	100 x 520 x 460		100 x 520 x 460		100 x 52	0 x 460
Dimensions OptiFill Bench dispenser		140 x 580 x 520		140 x 580 x 520		140 x 58	0 x 520	
Weight kg			19		20		20	C
* in depend	dence on the feedwate	er quality	** with sterilizing filter 0	.2 µm *** w	th OptiFill Disp	benser		
Article no.	System type* Standard	Article no.	System type Production unit + Wall dispenser*/**	Article no. Proc	em type duction unit + ch dispenser*		ypical applications	
18200001	OmniaPure	18200011	OmniaPure-W	18200021 Omi	niaPure-T	A	AS. IC. ICP. buffers and m	edia preparati

18200001	OmniaPure	18200011	OmniaPure-W	18200021	OmniaPure-T	AAS, IC, ICP, buffers and media preparation
18200002	OmniaPure UV	18200012	OmniaPure-W UV	18200022	OmniaPure-T UV	Ultra-trace analysis, ICP-MS, HPLC, TOC-analysis
18200003	OmniaPure UV/UF	18200013	OmniaPure-W UV/UF	18200023	OmniaPure-T UV/UF	Life science and microbiology, cell culture media
18200004	OmniaPure UV-TOC	18200014	OmniaPure-W UV-TOC	18200024	OmniaPure-T UV-TOC	Ultra-trace analysis, ICP-MS, HPLC, TOC-analysis
18200005	OmniaPure UV-TOC/UF	18200015	OmniaPure-W UV-TOC/UF	18200025	OmniaPure-T UV-TOC/UF	Life science and microbiology, cell culture media

\* filter cartridges and sterile filter capsule 0.2 μm included \*\*The Omnia production unit can either be installed on a bench, on a wall or under the bench.

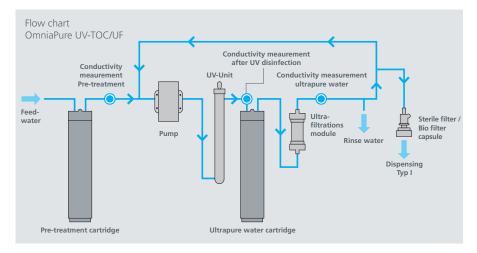

Accessorie	S
19200300	Wall mount Omnia
19200056	Disinfection kit Omnia
19200057	Disinfectant Omnia – 3 Pc./Pkg.

### OmniaTap The Allrounder. For $H_2O$ pure types I + II.

OmniaTap is the ideal system when both pure water and ultrapure water are required, but in relatively small amounts. The ability to provide both types from a single system results from the combination of ultramodern purification technologies. These also make it possible to connect the system directly to tap water. A press on the dispenser button activates dispensing of ultrapure water type I via the digital dispenser control. The recirculation of the pure water held in the installed 10 litre tank keeps it permanently at type II quality. The pure water tank has a second outlet for feeding downstream end users.

- OptiFill dispenser is standard
- Pretreatment set for direct connection to tap water
- 10-litres pure water tank
- Tank volume display in percent
- Simple and economical filter replacement
- Leakage sensor is standard
- Ready-to-use, including filter cartridges










Specifications	OmniaTap	OmniaTap UV	OmniaTap UV/UF
Туре II			
Pure water performance I/h at 15 °C	6 or 12	6 or 12	6 or 12
Conductivity µS/cm	0.067-0.1	0.067-0.1	0.067-0.1
Resistance M $\Omega$ x cm	15-10	15-10	15-10
Pure water tank pressurized outlet	optional	optional	optional
Туре І			
Conductivity µS/cm	0.055	0.055	0.055
Resistance M $\Omega$ x cm	18.2	18.2	18.2
TOC-value* ppb	5-10	1-5	1-5
Dispensing performance l/min.	up to 2	up to 2	up to 1.6
Endotoxins* EU/ml	-	-	< 0.001
Particles* */ml	< 1	< 1	< 1
Bacteria** CFU/ml	< 0.1	< 0.1	< 0.1
Feedwater requirements			
Tap water according to DIN 2000			
Feedwater temperature °C	+2 up to 35	+2 up to 35	+2 up to 35
Manganese and iron content mg/l	< 0.05	< 0.05	< 0.05
Free chlorine content mg/l	< 0.1	< 0.1	< 0.1
Silt density index (SDI)	max. 3	max. 3	max. 3
Technical data			
Operating pressure bar	2-6	2-6	2-6
Supply voltage Volt/Hz	90-240/50-60	90-240/50-60	90-240/50-60
Connected load kW	0.1	0.1	0.1
Connector size	3/4 "	3/4 "	3/4"
Ambient temperature °C	+2 up to +35	+2 up to +35	+2 up to +35
Dimensions*** W x H x D mm	390 x 720 x 615	390 x 720 x 615	390 x 720 x 615
Weight kg	20	21	21
* in dependence on the feedwater quality	** with sterilizing filter 0.2 $\mu m$	*** with OptiFill Dispenser	
Article no. System type* T	ypical applications	Accessories	

Article no.	System type*	lypical applications
18200051	OmniaTap 6	AAS, IC, ICP, buffers and media preparation
18200101	OmniaTap 12	AAS, IC, ICP, buffers and media preparation
18200052	OmniaTap 6 UV	Ultra-trace analysis, ICP-MS, HPLC, TOC
18200102	OmniaTap 12 UV	Ultra-trace analysis, ICP-MS, HPLC, TOC
18200053	OmniaTap 6 UV/UF	Life science and microbiology, cell culture media
18200103	OmniaTap 12 UV/UF	Life science and microbiology, cell culture media

Accessories	
19200300	Wall mount Omnia
19200056	Disinfection kit Omnia
19200057	Disinfectant Omnia – 3 pcs./pack
19200021	Pre-treatment unit OmniaTap –10"

 $\ast$  RO cartridge, ultrapure water cartridge, sterile filter capsule 0.2  $\mu m$ , sterile overflow and sterile vent filter included

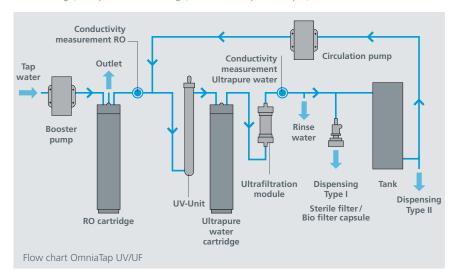

### OmniaLab<sup>ED+</sup> The big one. For $H_2O$ pure types I + II.

OmniaLab<sup>ED+</sup> is the system of choice when both pure water and ultrapure water are needed for the entire laboratory. The system complies with international water standards such as ASTM, ISO 3696 and CLSI. The economy of it is maximized by the inclusion of a continuously self-regenerating electrodeionizer, without having to give any demanding analytical applications a pass. Further to this, the OmniLab<sup>ED+-</sup> system holds 100 liters of pure water Type II ready for withdrawal in a storage tank with quality recirculation. It is so predestined for supplying autoclaves or lab washing machines and the dispensing of Type 1 tultra pure water for analytical and bioscience applications.

- OptiFill dispenser is standard
- Continuous residual salts removal by electro-deionization
- 100 litre storage tank with recirculation and pressure outlet
- Tank volume display in percent
- Tank volume can be modularly increased
- Simple, cost-effective filter replacement
- Leakage sensor is standard







Flexible on a work surface



Tank fits space . savingly under the bench-top



Specifications	OmniaLab <sup>ED+</sup> 20	OmniaLab <sup>ED+</sup> 40	OmniaLab <sup>ED+</sup> 70	
Туре II				
Pure water performance l/h at 15 °C	20	40	70	
Conductivity µS/cm	0.067-1	0.067-1	0.067-1	
Resistance M $\Omega$ x cm	15–1	15-1	15–1	
Silicate removal* %	99.9	99.9	99.9	
Pure water tank pressurized outlet	optional	optional	optional	
Туре I				
Conductivity µS/cm	0.055	0.055	0.055	
Resistance M $\Omega$ x cm	18.2	18.2	18.2	
TOC-value* ppb (with UV-unit)	1-5	1-5	1-5	
Dispensing performance dispenser l/min.	up to 2	up to 2	up to 2	
Particles**/ml	< 1	< 1	< 1	
Bacteria** CFU/ml	< 0.1	< 0.1	< 0.1	
Feedwater requirements Softened water according to DIN 2000				
-	2	2	2	
Feedwater temperature °C	+ 2 up to 35	+ 2 up to 35	+2 up to 35	
Manganese and iron content mg/l	< 0.05	< 0.05	< 0.05	
Free chlorine content mg/l				
Silt density index (SDI)	max. 3	max. 3	max. 3	
Technical data				
Operating pressure bar	2-6	2-6	2-6	
Supply voltage Volt/Hz	90-240/50-60	90-240/50-60	90-240/50-60	
Connected load kW	0.25	0.25	0.25	
Connector size	3/4 "	3/4 "	3/4 "	
Ambient temperature °C	+2 up to +35	+2 up to +35	+2 up to +35	
Dimensions Tower*** W x H x D mm	511 x 1520 x 575	511 x 1520 x 575	511 x 1520 x 575	
Dimensions Base cabinet tank mm	511 x 800 x 575	511 x 800 x 575	511 x 800 x 575	
Dimensions base capinet tank min			511 / 000 / 5/ 5	

\* in dependence on the feedwater quality


\*\* with sterilizing filter 0.2 µm


\*\*\* with OptiFill Dispenser

Article no.	System type*	Typical applications
18700020	OmniaLab <sup>ED+</sup> 20	Feedwater for autoclaves and laboratory washers
18700040	OmniaLab <sup>ED+</sup> 40	Feedwater for autoclaves and laboratory washers
18700070	OmniaLab <sup>ED+</sup> 70	Feedwater for autoclaves and laboratory washers

\* RO cartridge, ultrapure water cartridge, sterile filter capsule 0.2  $\mu$ m, sterile overflow and sterile vent filter + CO<sub>2</sub> absorber included

Accessories	
16125000	Water softener MixMulti 32
19200021	Pre-treatment unit OmniaLab – 10"
19200050	UV Flow through disinfection – 254 nm
19200052	UV Unit for TOC reduction – 254 nm
16561201	External pressure booster pump SC 3000

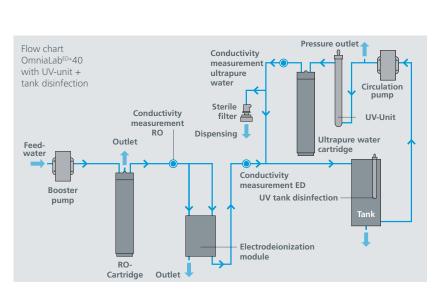



### OmniaLab<sup>ED</sup> The efficient one. For $H_2O$ pure type II.

OmniaLab<sup>ED</sup> is the efficient solution when high quality pure water Type II is required for the complete lab supply. It is compliant with international water standards, such as ASTM, ISO 3696, CLRW (CLSI), and the combination with continual self-regenerating electro-deionization brings maximized economy. Further to this, the OmniaLab<sup>ED</sup> system holds 100 liters of pure water in a storage tank with quality recirculation, ready to supply lab equipment. OmniaLab<sup>ED</sup> is the efficient one for supplying autoclaves, lab machines and ultra-pure water systems.

- OptiFill dispenser is standard
- Continuous residual salts removal by electro-deionization
- 100 litre storage tank with recirculation and pressure outlet
- Tank volume display in percent
- Tank volume can be modularly increased
- Simple, cost-effective filter replacement
- Leakage sensor is standard







Easy water dispensing





savingly under the bench-top





Specifications	OmniaLab <sup>ED</sup> 20	OmniaLab <sup>ED</sup> 40	OmniaLab <sup>ED</sup> 70
Туре II			
Pure water performance l/h at 15 °C	20	40	70
Conductivity* µS/cm	0.1-1	0.1-1	0.1-1
Resistance* M $\Omega$ x cm	10-1	10-1	10-1
TOC-value* ppb	< 30	< 30	< 30
Silicate removal* %	> 99	> 99	> 99
Dispensing performance dispenser l/min.	up to 2	up to 2	up to 2
Particles**/ml	< 1	< 1	< 1
Bacteria** CFU/ml	< 0.1	< 0.1	< 0.1
Pure water tank pressurized outlet	optional	optional	optional
Feedwater requirements			
Softened water according to DIN 2000			
Feedwater temperature °C	+2 up to 35	+2 up to 35	+2 up to 35
Manganese and iron content mg/l	< 0.05	< 0.05	< 0.05
Free chlorine content mg/l	< 0.1	< 0.1	< 0.1
Silt density index (SDI)	max. 3	max. 3	max. 3
Technical data			
Operating pressure bar	2-6	2-6	2-6
Supply voltage Volt/Hz	90-240/50-60	90-240/50-60	90-240/50-60
Connected load kW	0.25	0.25	0.25
Connector size	3/4 "	3/4"	3/4 "
Ambient temperature °C	+2 up to +35	+ 2 up to + 35	+2 up to +35
Dimensions Tower*** W x H x D mm	511 x 1520 x 575	511 x 1520 x 575	511 x 1520 x 575
Dimensions Base cabinet tank mm	511 x 800 x 575	511 x 800 x 575	511 x 800 x 575
Weight kg	41	41	43
* in dependence on the feedwater quality	**with sterilizing filter 0.2 up	***with OntiFill Dispenser	

\* in dependence on the feedwater quality \*\* with sterilizing filter 0.2 µm \*\*\* with OptiFill Dispenser

Article no.	System type*	Typical applications	Accessories	;
18700021 OmniaLab <sup>ED</sup> 20	Feedwater for autoclaves, laboratory washers and	16125000	Water softener MixMulti 32	
		ultrapure water systems	19200020	Pre-treatment unit OmniaLab – 10"
18700041	OmniaLab <sup>ED</sup> 40	Feedwater for autoclaves, laboratory washers and ultrapure water systems	19200050	UV Tank disinfecting unit 254 nm
18700071 OmniaLab <sup>ED</sup> 70	671 Ompial abEP70 Feedwater for autoclaves, laboratory washers and	19200051	UV Flow through disinfection 254 nm	
		ultrapure water systems	16561201	External pressure booster pump SC 3000

\* RO cartridge, sterile filter capsule 0.2  $\mu$ m, sterile overflow and sterile vent filter + CO<sub>2</sub> absorber included

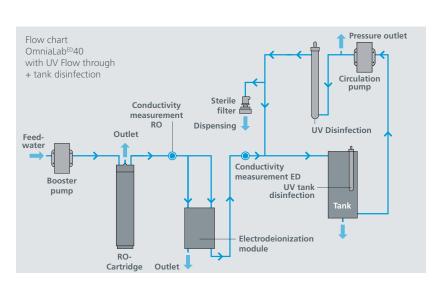



Omnia pure and ultrapure water systems. Convenient. Compact. Adaptable.

### OmniaLab<sup>UP</sup> The constant one. For $H_2O$ pure type II.

OmniaLab<sup>UP</sup> is the system of choice when you need a constant supply of high-quality water in laboratories. For this, OmniaLab<sup>UP</sup> holds 100 litres of type II pure water in reserve in a storage tank with quality recirculation. It is an optimal supplier to autoclaves, lab rinsing machines and ultrapure water systems. The water produced conforms to international medical technology water standards such as ASTM, ISO 3696 and CLRW (CLSI).

- OptiFill Dispenser is standard
- 100 I tank with quality recirculation and pressure outlet
- Tank volume display in percent
- Tank volume can be modularly increased
- Simple, cost-effective filter replacement
- Leakage sensor is standard







Flexible on a work surface



Tank fits spacesavingly under the bench top




Specifications	OmniaLab <sup>u</sup> ²20	OmniaLab <sup>up</sup> 40	
Туре II			
Pure water performance l/h at 15 °C	20	40	
Conductivity µS/cm	0.067-0.1	0.067-0.1	
Resistance M $\Omega$ x cm	15-10	15-10	
Dispensing performance dispenser l/min.	up to 2	up to 2	
Pure water tank pressurized outlet	optional	optional	
Particles*/ml	< 1	< 1	
Bacteria* CFU/ml	< 0.1	< 0.1	
Feedwater requirements			
Softened or hardness-stabilized water according to DIN 2000			
Feedwater temperature °C	+2 up to 35	+2 up to 35	
Manganese and iron content mg/l	< 0.05	< 0.05	
Free chlorine content mg/l	< 0.1	< 0.1	
Silt density index (SDI)	max. 3	max. 3	
Technical data			
Operating pressure bar	2-6	2-6	
Supply voltage Volt/Hz	90-240/50-60	90-240/50-60	
Connected load kW	0.1	0.1	
Connector size	3/4 "	3/4 "	
Ambient temperature °C	mbient temperature °C +2 up to +35 °C		
Dimensions Tower** W x H x D mm	511 x 1520 x 575	511 x 1520 x 575	
Dimensions Base cabinet tank mm	511 x 800 x 575	511 x 800 x 575	
Weight kg	40	40	

 $\ast$  with sterilizing filter 0.2  $\mu m$ \* \* with OptiFill Dispenser

Article no.	System type*	Typical applications	Accessories	5
18600020	OmniaLab <sup>u</sup> ²20	Feedwater for autoclaves and laboratory washers	19200020	Pre-treatment unit OmniaLab – 10"
18600040	OmniaLab <sup>up</sup> 40	Feedwater for autoclaves and laboratory washers	19200050	UV tank disinfection unit 254 nm
* RO cartridge, pure water cartridge, sterile filter capsule 0.2 µm, sterile overflow and sterile			19200051	UV Flow through disinfection 254 nm

ap 0.2 µm, vent filter +  $CO_2$  absorber included.

Accessories	
19200020	Pre-treatment unit OmniaLab – 10"
19200050	UV tank disinfection unit 254 nm
19200051	UV Flow through disinfection 254 nm
16561201	External pressure booster pump SC 3000

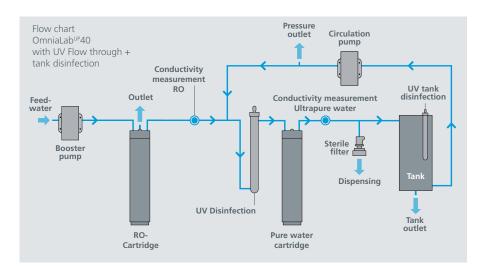

### OmniaLab<sup>DS</sup> The reliable one. For H<sub>2</sub>O pure type II + CLRW (CLSI).

When safety is first priority and the quality of the purification decides the quality of results, then the OmniaLab<sup>DS</sup> system is the perfect solution. Even for large pure water quantities of up to 80 l/h, OmniaLab<sup>DS</sup> guarantees international water standards compliance. The combination of regenerative polishing cartridge and an optional emergency supply makes this system extremely reliable for supplying clinical analytical systems, as well as for feeding water to steam sterilizers and washer-disinfectors.

- OptiFill Dispenser is standard
- 100 I tank with quality recirculation and pressure outlet
- Tank volume display in percent
- Tank volume can be modularly increased
- Simple, cost-effective filter replacement
- Leakage sensor is standard
- Emergency supply (optional)
- Degassing unit (optional)





Easy water dispensing

Flexible on a work surface



savingly under the bench top




Specifications	OmniaLab <sup>DS</sup> 20	OmniaLab <sup>DS</sup> 40	OmniaLab <sup>DS</sup> 60	OmniaLab <sup>DS</sup> 80
Type II + CLRW (CLSI) DIN EN 285 + ISO EN 15883				
Pure water performance I/h at 15 °C	20	40	60	80
Conductivity µS/cm	0.1-1.0	0.1-1.0	0.1-1.0	0.1-1.0
Resistance M $\Omega$ x cm	10-1	10-1	10-1	10-1
Dispensing performance dispenser l/min.	up to 2	up to 2	up to 2	up to 2
Pure water tank pressurized outlet	optional	optional	optional	optional
Particles*/ml	< 1	< 1	< 1	< 1
Bacteria* CFU/ml	< 0.1	< 0.1	< 0.1	< 0.1
Feedwater requirements				
Softened or hardness-stabilized water according to DIN 2000				
Feedwater temperature °C	+2 up to 35			
Manganese and iron content mg/l	< 0.05	< 0.05	< 0.05	< 0.05
Free chlorine content mg/l	< 0.1	< 0.1	< 0.1	< 0.1
Silt density index (SDI)	max. 3	max. 3	max. 3	max. 3
Technical data				
Operating pressure bar	2-6	2-6	2-6	2-6
Supply voltage Volt/Hz	90-240/50-60	90-240/50-60	90-240/50-60	90-240/50-60
Connected load kW	0.1	0.1	0.1	0.1
Connector size	3/4"	3/4 "	3/4 "	3/4"
Ambient temperature °C	+2 up to +35			
Dimensions Tower** W x H x D mm	511 x 1520 x 575			
Dimensions Base cabinet tank mm	511 x 800 x 575			
Weight kg (without polishing cartridge)	39	39	40	40

\* with sterilizing filter 0.2  $\mu$ m \*\* with OptiFill Dispenser

Article no.	System type	Typical applications
18800020	OmniaLab <sup>DS</sup> 20	Feedwater for analyzers, autoclaves and laboratory washers
18800040	OmniaLab <sup>DS</sup> 40	Feedwater for analyzers, autoclaves and laboratory washers
18800060	OmniaLab <sup>DS</sup> 60	Feedwater for analyzers, autoclaves and laboratory washers
18800080	OmniaLab <sup>DS</sup> 80	Feedwater for analyzers, autoclaves and laboratory washers

Accessories	5
19200020	Pre-treatment unit OmniaLab – 10"
19200050	UV tank disinfection unit 254 nm
19200051	UV Flow through disinfection 254 nm
12280050	Replacement/second polishing cartridge type DS 2800 RV
19200040	Emergency supply
19200041	Degassing unit
16561201	External pressure booster pump SC 3000



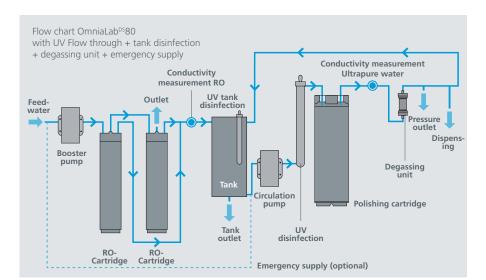

# $\begin{array}{l} OmniaLab^{RO}\\ The big one.\\ For H_2O pure type III. \end{array}$

OmniaLab<sup>RO</sup> fulfils your requirement when you have a needof a constant large volume of reverse osmosis water. For this, OmniaLab<sup>RO</sup> holds 100 litres in reserve in a storage tank. It is an optimal supplier to autoclaves, lab rinsing machines, air humidifiers and ultrapure water systems.

- OptiFill Dispenser is standard
- With 100 I pure water tank
- Tank volume display in percent
- Tank volume can be modularly increased
- Leakage sensor is standard







Flexible on a work surface



Tank fits spacesavingly under the bench top




Specifications	OmniaLab <sup>RO</sup> 20	OmniaLab <sup>RO</sup> 40	OmniaLab <sup>₀</sup> 60	OmniaLab <sup>RO</sup> 80
Type III				
Pure water performance I/h at 15 °C	20	40	60	80
RO membrane retention rate in % (ions. germs and bacteria)	> 98	> 98	> 98	> 98
Feedwater requirements				
Softened or hardness-stabilized water according to DIN 2000				
Feedwater temperature °C	+2 up to 35	+2 up to 35	+2 up to 35	+2 up to 35
Manganese and iron content mg/l	< 0.05	< 0.05	< 0.05	< 0.05
Free chlorine content mg/l	< 0.1	< 0.1	< 0.1	< 0.1
Silt density index (SDI)	max. 3	max. 3	max. 3	max. 3
Technical data				
Operating pressure bar	2-6	2-6	2-6	2-6
Supply voltage Volt/Hz	90-240/50-60	90-240/50-60	90-240/50-60	90-240/50-60
Connected load kW	0.1	0.1	0.1	0.1
Connector size	3/4"	3/4 "	3/4 "	3/4"
Ambient temperature °C	+2 up to +35	+2 up to +35	+2 up to +35	+2 up to +35
Dimensions Tower* W x H x D mm	511 x 1520 x 575	511 x 1520 x 575	511 x 1520 x 575	511 x 1520 x 575
Dimensions Base cabinet tank mm	511 x 800 x 575	511 x 800 x 575	511 x 800 x 575	511 x 800 x 575
Weight kg	38	38	40	40

\* with OptiFill Dispenser

Article no.	System type	Typical applications
18500020	OmniaLab <sup>RO</sup> 20	Feedwater for autoclaves and laboratory washers, ultrapure water systems and air humidifiers
18500040	OmniaLab <sup>®0</sup> 40	Feedwater for autoclaves and laboratory washers, ultrapure water systems and air humidifiers
18500060	OmniaLab <sup>®0</sup> 60	Feedwater for autoclaves and laboratory washers, ultrapure water systems and air humidifiers
18500080	OmniaLab <sup>R0</sup> 80	Feedwater for autoclaves and laboratory washers, ultrapure water systems and air humidifiers

Accessories	
19200020	Pre-treatment unit OmniaLab – 10"
19200050	UV tank disinfection unit 254 nm
16561201	External pressure booster pump SC 3000

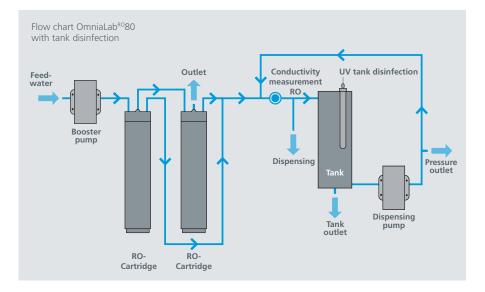

## stakpure

**stakpure GmbH** Auf dem Kesseling 11 D 56414 Niederahr Phone: +49 (0) 2602 10673-0 Fax: +49 (0) 2602 10673-200 info@stakpure.de **www.stakpure.de** 





We are certified according to ISO 9001: 2015

Is reliable and economic preparation of pure and/or ultrapure water a topic for you? Just call us!

info@stakpure.de www.stakpure.de

Retailer panel

Subject to changes and printing errors.